

Thermometer Calibration Guide

NIST Reference
Thermometer






Dial Bimetal Coil
Thermometer ‡



Calibration for cold process use ice water method

Calibration for hot process use boiling water method

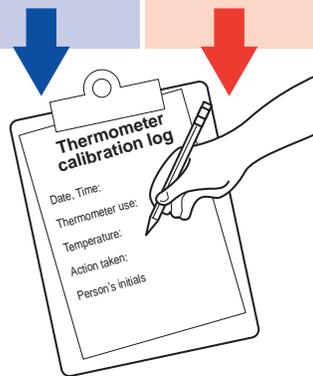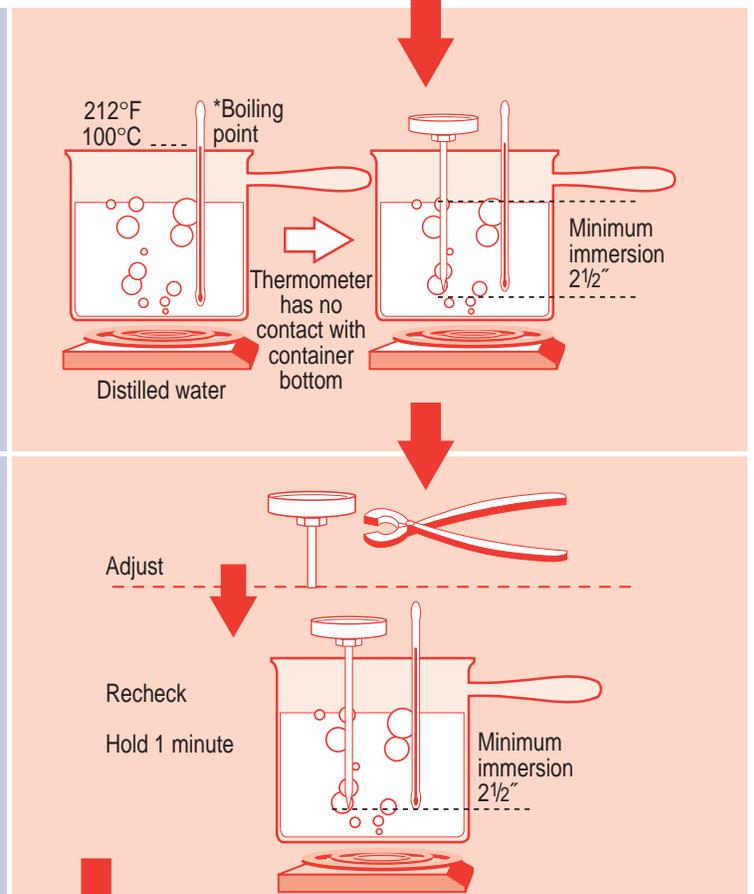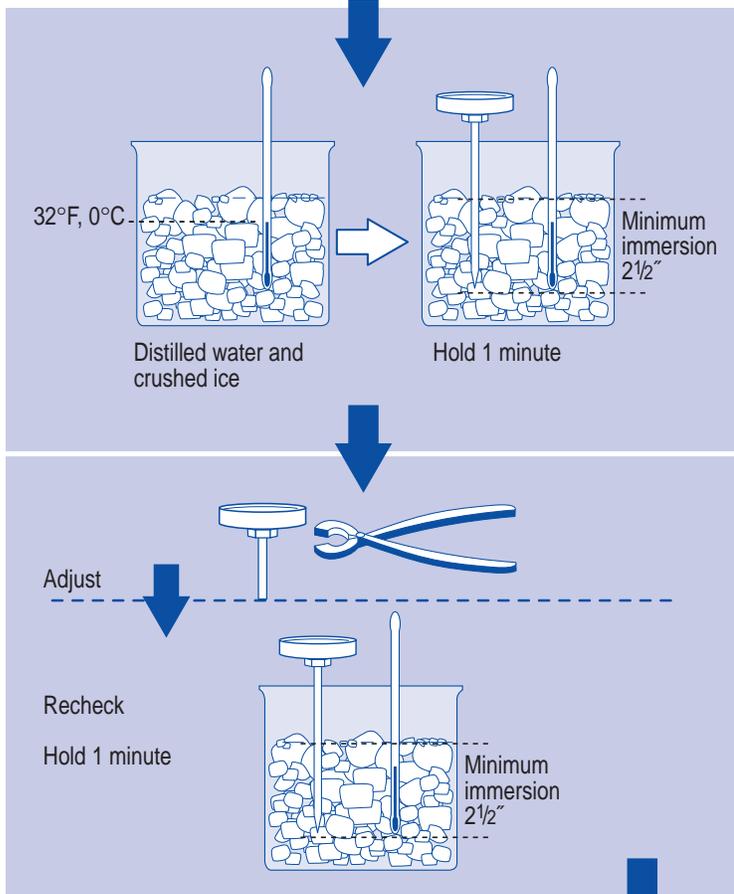

‡ Check operations manual for calibration procedure for other thermometer types.

*Boiling point temperature varies with altitude. Verify using an altitude temperature chart.

N.C. Flores and E.A.E. Boyle, Department of Animal Sciences and Industry
Kansas State University, Weber Hall, Manhattan, KS 66506